

turbomedorthotics.com

XTERN FOOT DROP ORTHOTIC - SIZING CHART -

US SHOE SIZE			KIT SIZE SELECTION			
			PRODUCT: 100100-SA-L	PRODUCT: 100100-SA-M	PRODUCT: 100100-SA-S	PRODUCT: 100100-SA-P
	\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\	1/100	100100 SA E	100100 SA 14	100100 3A 3	100100 SA 1
MEN	WOMEN	KIDS	LARGE	MEDIUM	SMALL	PEDIATRIC
16			X			
15.5			X			
15			X			
14.5			X			
14			X			
13.5			X			
13			X	SI	SELECT BEST SIZE FROM	
12.5 12			X X	PATIENT FOOT WIDTH		
11.5			X			
11			X			
10.5	11.5		X	X		
10	11			X		
9.5	10.5			X		
9	10			X		
8.5	9.5			X		
8	9	8 Y		X	X	
7.5	8.5	7.5 Y		X	X	
7	8	7 Y			X	
6.5	7.5	6.5 Y			X	
6	7	6 Y			X	
5.5 5	6.5 6	5.5 Y 5 Y			X	
4.5	5.5	4.5 Y			X X	
4	5	4.5 T			X	
3.5	4.5	3.5 Y			X	
3	4	3 Y			X	X
2.5	3.5	2.5 Y			X	X
		2 Y				X
		1.5 Y				X
		1 Y				X
		13 C				X
		12.5 c 12 c				X X
		12 C				X
		10.5 c				X
		10.5 C				X
		9.5 c				X

Y: YOUTH SHOE SIZE (6-10 YEARS) C: CHILDREN SHOE SIZE (1-5 YEARS)



EASILY TRANSFERABLE!






XTERN FOOT DROP BRACE - DORSIFLEXION ASSIST

The **XTERN** is the only Dynamic AFO totally affixed outside the shoe to maximize comfort, prevent skin breakdown and rubbing injuries to the foot. Its flexibility helps keep maximal ankle range of motion and calf muscle strength.

The XTERN AFO acts as a Preloaded Exo-Skeleton Spring, and transfers dorsiflexion forces directly to footwear to keep foot at 90deg.

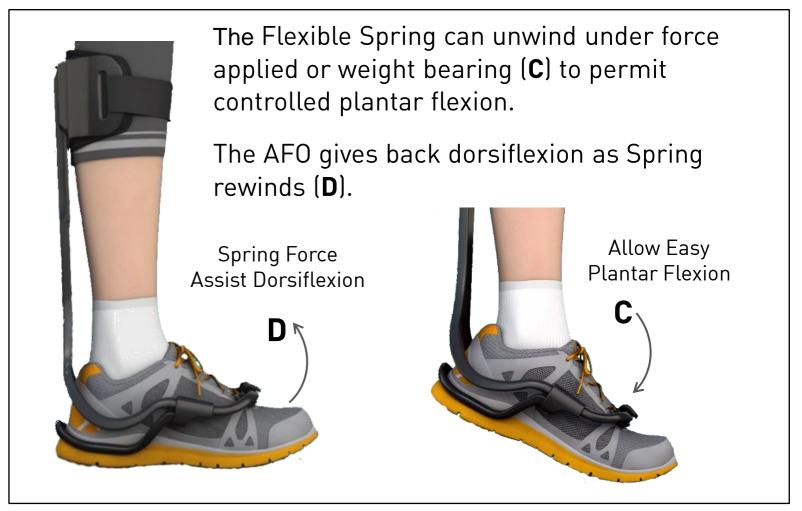

*HCPCS Code L1951 PDAC VALIDATED



L1951: Ankle foot orthosis, spiral, (institute of rehabilitative medicine type), plastic or other material, prefabricated, includes fitting and adjustment.

*Suggested L Codes: The responsibility for accurate coding lies with the patient care facility that selects the product, fits the patient, and bills for the service.

CLINICAL INDICATIONS

- Drop Foot & Dorsiflexion Weakness
- Peroneal Nerve Injury
- Charcot Marie Tooth (CMT)
- Stroke (CVA)
- Multiple Sclerosis (MS)
- Cerebral Palsy (CP)
- Guillain-Barre Syndrome (GBS)
- Motor Neuropathy
- Motor Neurone Disease (MND)

CLINICAL LIMITATIONS

- Inappropriate Footwear
- Gross Fixed Deformities of Foot and Ankle
- Severe Spasticity
- Quadriceps weakness
- Severe Proximal weakness
- Crouch gait

WE RECOMMEND THE QUALIFIED HEALTH CARE PROVIDER ASSESS THE PATIENT WITH AN AT-X ASSESSMENT TOOL.

> TurboMed Orthotics Inc. 240 Sydney (Suite 101) St-Augustin-de-Desmaures, QC G3A 0P2 CANADA

1 888 778-8726

info@turbomedorthotics.com

